



Rapidox 3100A Oxygen / CO₂ Dual Gas Analyser

Instruction Manual

Revision 1.0

Cambridge Sensotec Limited
31 Elizabeth Court
St Ives
CAMBS
PE27 5BQ

Tel. +44 (0)1480 385812
Fax +44 (0)1480 352529
Mobile (07866) 624236
Sales@Cambridge-Sensotec.co.uk

Declaration of Conformity

Manufacturer: Cambridge Sensotec Limited
31 Elizabeth Court
St. Ives
CAMBS PE27 5BQ
England

Product Names: Rapidox portable oxygen gas analyser


Model Numbers: RX2100 RX3100

Conform to the following specifications:

EMC: EN 61326:1998 Electrical equipment for measurement,
control and laboratory use

Declaration

I declare that the above products conform to the applicable requirements of the LVD Directive 73/23/EEC and the EMC Directive 89/336/EEC and is CE marked accordingly.

Signature: 

Name: Dr. Mark Swetnam

Title: Managing Director

Company: Cambridge Sensotec Limited

Date: 1st Jan 2008

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

Contents

1.	Introduction	1
2.	Features	1
3.	Specification	2
3.1	Rapidox 3100 Dimensions	2
3.2	Response Time, Accuracy and Precision	2
3.3	Display.....	2
4.	Sensor Location.....	3
4.1	Oxygen Calibration	3
4.2	Operating Temperature.....	3
4.3	Outputs	4
5.	Technical Specification	4
6.	Precautions	5
7.	Rapidox Operating Instructions.....	5
7.1	The Rapidox Analyser - Menu System	6
7.2	Rapidox Calibration – Oxygen Sensor	9
7.3	Selecting the Calibration Gases.....	10
7.4	Cleaning the Sensor.....	10
7.5	Oxygen Sensor Range	11
7.6	Alarms	11
7.7	Analogue Outputs.....	12
7.8	Setting the Display Units.....	12
7.9	Setting the Display Options.....	13
7.10	Operating Mode.....	13
7.11	Internal Pressure Sensor	14
7.12	Pressure Mode	15
7.13	Setting the Baud Rate	15
7.14	Load Defaults	16
7.15	Type K Thermocouple.....	16
7.16	RS232 / RS485 Port	16
7.16.1	RS232 Protocol.....	16
7.16.2	RS485 Protocol.....	17
8.	Rapidox Software Instructions	18
8.1	Software Installation.....	18
8.2	Getting Started.....	18
8.3	On-Screen Help	19
8.4	Configuration Page.....	19
8.5	Reconfiguring the Analyser.....	20
8.5.1	Config 1 Screen	21
8.5.2	Config 2 Screen	22
8.6	On-Screen LCD.....	24
8.7	Remote Calibrating and Cleaning	24
8.8	Setting Analyser Date and Time	24
9.	Rapidox Data-Logging Software.....	25
9.1	Introduction	25
9.2	Setting up the Data Logger.....	25
9.3	Running the Data Logger	26
9.4	Auto Date Stamped Files.....	26
9.5	Live Time Graphing Screen	27

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

9.6	Main Graph Window.....	28
9.7	Plot Colours.....	28
9.8	Graph Titles and Labels.....	29
9.9	Plot Co-ordinates.....	29
9.10	Last data point.....	29
9.11	Using the Cursor.....	30
9.12	Zooming.....	30
9.13	Y-Axis Graph Units.....	30
9.14	Oxygen Scale.....	30
9.15	Second Y Axis.....	30
9.16	Loading an Old Run.....	31
9.17	Printing Graphs.....	31
9.18	Data Logging in the Background.....	31
9.19	Pausing the Data Logging.....	31
9.20	Changing the Data Logging Parameters Mid-run.....	31
9.21	Working with Spreadsheets.....	32
9.22	Disaster Recovery.....	32
9.23	Diagnostics.....	32
10.	Troubleshooting.....	33
11.	Warranty.....	34
11.1	Conditions of Warranty:.....	34

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

1. Introduction

The Rapidox 3100 dual gas analyser allows fast and accurate oxygen analysis over the full oxygen range (10e⁻²⁰ppm to 100% O₂) and CO₂ (0-5, 0-10, 0-20% range selected at the time of order). The Rapidox 3100 analyser provides continuous on-line gas analysis, with a typical response time of 5 seconds for a 90% response to a step change in oxygen compositions and approximately 30 seconds for a 90% step change in CO₂.

The Rapidox 3100 is a fully integral unit complete with a powerful yet quiet linear piston pump to provide gas sampling in the range 0.1 to 2 litres per minute.

The oxygen sensor head is located inside the analyser and comprises a zirconia ceramic tube that needs to be heated to 650°C before it will conduct oxygen ions. The analyser supplies heat to the sensor, which is controlled very accurately by a regulated power supply incorporated in the instrument. An internally mounted pressure sensor compensates for any fluctuations in pressure or vacuum caused by differing flow conditions.

The Co₂ sensor is based on infra-red cell technology which gives extremely stable and accurate readings over a period of many years. The cell has a life-expectancy in excess of ten years and is supplied fully calibrated. No further adjustments are required.

The analyser is packed with features including fully programmable alarm circuits, programmable analogue outputs (0-5V and 4-20mA), easy oxygen calibration (user selectable gases), RS232 communications and a full set of communications / data-logging software.

2. Features

- Bench mounted gas sampling oxygen & CO₂ gas analyser
- Continuous gas sampling via powerful yet quiet internally located linear piston pump
- Flow rate controlled by needle valve / flow gauge on front panel
- Fast measurement response (typically 5 seconds for a 90% change in oxygen)
- Full measurement range available (10e⁻²⁰ ppm to 100% oxygen & 0-5, 0-10, 0-20% CO₂)
- High accuracy maintained throughout the measurement range. Accuracy ± 1% of the actual measured oxygen with a precision ± 0.5%, and +/- 1.5% full scale accuracy for CO₂ measurements.
- Nernst mode of operation for ultra low oxygen concentrations

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

- Independent type K thermocouple fitted as standard. Range 0-1000°C
- Oxygen sensor easy to calibrate by the user using ANY TWO gases (air is usually chosen for convenience).
- Oxygen sensor life expectancy typically 35,000 hours. Ten years for CO₂
- Large back-lit LCD display showing % oxygen (selectable notation), % CO₂, temperature & pressure.
- RS232, RS485, 0-5V or 4-20mA current loop outputs (both user programmable)
- Windows data logging software with MS-Excel compatible graphing included
- Fully programmable alarms (low and high condition) with outputs and visual / audible warning
- Unique oxygen sensor cleaning facility which can be operated at any time during use

3. Specification

3.1 *Rapidox 3100 Dimensions*

The unit weighs approximately 5kg and is fitted with adjustable rubber feet. The unit is mains powered (110/240V 50/60Hz) and is supplied with mains cable. Case dimensions W=350mm; D=263mm; H=150mm.

3.2 *Response Time, Accuracy and Precision*

Oxygen sensor response time is typically 5 seconds for a 90% response involving a step change in composition. A change between 21% and 100% can be recorded in less than 4 seconds depending on sampling flow-rates. The CO₂ sensor has a typical response time of thirty seconds for a 90% response involving a step change in composition. High oxygen accuracy is maintained between calibration points. Accuracy better than $\pm 1\%$ of the actual measured oxygen content with a precision better than $\pm 0.5\%$. Outside calibration range accuracy is typically $\pm 2.5\%$. The CO₂ sensor accuracy is quoted as $\pm 1.5\%$ of full scale.

3.3 *Display*

The analyser has a 2-line 16x2, 9mm character, back-lit liquid crystal display (LCD) , whose data update rate is user-programmable.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

The LCD displays four significant figures of oxygen on line one. The display notation (percent, ppm, exponential or 'automatic') is user selectable. Values of oxygen below 10⁻¹ppm are always displayed using exponential notation. The working range is 1 x 10⁻²⁰ppm (=1 x 10⁻²¹%) to 100%.

The percent CO₂ reading is displayed on the second line of the display and is to three significant figures in percent.

The temperature display range is 0 to 1000°C (type 'K' thermocouple).

The internal pressure sensor output can be displayed as an alternative to the thermocouple. Range is +/- 1000mbar.

4. Sensor Location

The sensors are located inside the analyser and gas is drawn in using a top-of-the-range Medo linear-motor-driven free piston vacuum pump manufactured by Nitto; a world leader in pump technology. The pumps are exceptionally quiet (40 dB/m or less). The gas is sampled using flexible tubing that connects to the front panel via push fit pneumatic couplings. The flow rate is controlled using a flow gauge / needle valve on the front panel and is adjustable from 0 to 4 litres per minute. Oxygen sensor life expectancy is in excess of 35,000 hours and the sensor can be replaced by a skilled person. The CO₂ sensor is built on an integral card and has a life expectancy in excess of ten years.

4.1 *Oxygen Calibration¹*

The simple and fully flexible calibration procedure requires two calibration gases (ambient air 20.95% is normally used as calibration gas no. 1). The calibration gas compositions are user-selectable and programmed into the Rapidox via the keypad menu or the RS232 link and configuration software. Factory pre-sets can be reloaded to allow the unit to be 'rescued' from a failed calibration. The Rapidox is calibrated using the keypad on the front panel. The LCD changes to calibrate mode to inform the user of progress.

4.2 *Operating Temperature*

Gas temperature entering the analyser must not exceed 55°C. The tubing inside the analyser is rated to 200°C. The Rapidox unit normal operating temperature is 5-35°C.

¹ No calibration is required for the CO₂ sensor which is factory calibrated and fixed for the life of the cell.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

4.3 Outputs

The RS232 serial port outputs on demand values for oxygen (ppm), temperature (Celsius), time (hh:mm:ss) and date (dd/mm/yy). This data can be downloaded and logged using the software provided.

Standard 0-5V and 4-20mA analogue outputs are available on the rear panel for O₂ CO₂ and temperature, as are 5V (logic level) O₂ alarm signals (High and Low conditions). These outputs are fully user-programmable via the front keypad or RS232 link and the supplied configuration software.

5. Technical Specification

Rapidox 3100 Analyser	
Voltage (must be specified)	110 OR 220V / 240V ac 50/60 Hz
Analyser dimension	350mm X 263mm X 150mm
Weight	5 kg
Display	16 X 2 character (9mm) back lit
Warm up time	10 minutes at 20°C
Normal operating temperature	5-35°C
Outputs O ₂ & CO ₂ OR temperature OR pressure	0-5V logarithmic (user-programmable) into minimum 5kΩ
O ₂ & CO ₂ OR temperature OR pressure	4-20mA current loop (user-programmable) into maximum 500Ω
All data and parameters	RS232 or RS485 - data streamed on demand
Oxygen Calibration	Requires 2 user-selectable gas compositions (air is default plus another)
CO ₂ Calibration	Factory set
Thermocouple	Type K fitted to standard compensated plug Range 0-1000°C accuracy ± 1°C
Sample Pump	Mains type linear piston vacuum pump
Maximum Free Air Displacement	7 L.min ⁻¹ (0.28 Cfm)
Noise Level	40 dB (max) at 1 meter
Max. gas temperature on input	55°C
Sensor Life expectancy	typically 35,000 hours for oxygen & greater than ten years for CO ₂
Range of measurement	10e ⁻²⁰ ppm to 100% O ₂ 0-5, 0-10, 0-20% range (as ordered)
Response time (@ gas flow rate 1l.min ⁻¹)	approximately 5 secs for a 90% step change in oxygen approximately 30 seconds for a 90% step change in CO ₂
Accuracy	± 1% of the actual oxygen concentration ± 1.5% full scale reading of CO ₂
Precision of measurement	± 0.5% of the reading

6. Precautions

Make sure you read and understand these instructions and keep them safe for later use. The unit should not be exposed to extreme temperatures $< -5^{\circ}\text{C}$ or $> 60^{\circ}\text{C}$. Normal operating temperature is $5\text{-}35^{\circ}\text{C}$. Avoid direct sunlight. Do not use liquid cleaners, aerosols or solvents to clean the case. Use a damp cloth for cleaning. Do not use this equipment near water. Avoid touching the LCD display as this may cause permanent damage. Make sure the rear ventilation slots and the fan on the rear panel are free of obstruction.

Always make sure you use an in-line particle filter when operating this equipment as the CO₂ detector is very sensitive to dirt contamination.

This unit has been designed for strictly non-condensing conditions. Humid gas must be dried before entering the analyser to prevent condensation on the CO₂ cell. In practice this means lowering the dewpoint of the gas to below the temperature of the sensor.

There are no user serviceable parts in this unit. Do not attempt to repair yourself. Refer all servicing to qualified Cambridge Sensotec personnel.

7. Rapidox Operating Instructions

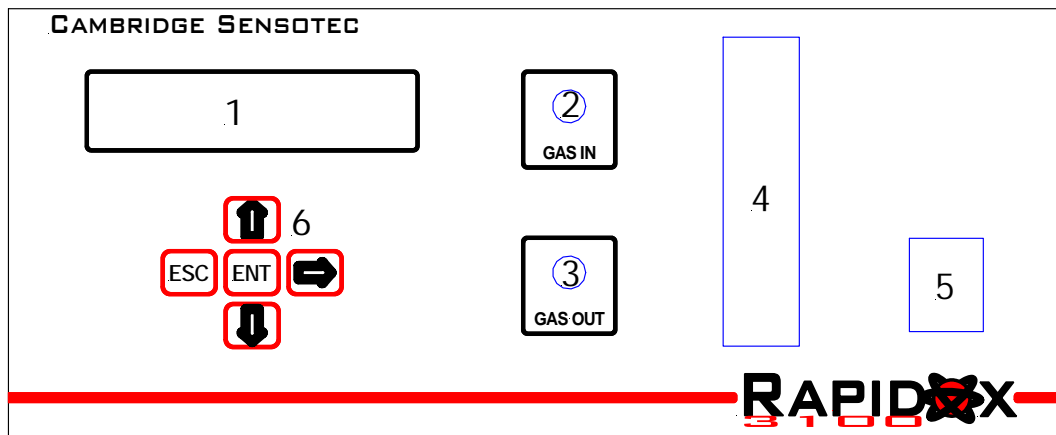


Figure 1: Rapidox 3100 front panel. The numbers refer to the instructions below.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

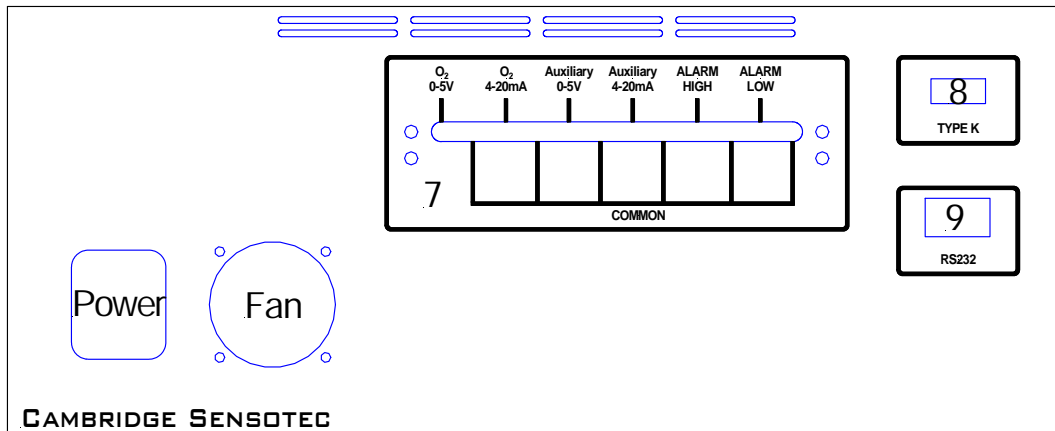


Figure 2: Rapidox 3100 rear panel. The numbers refer to the instructions below.

Ensure that the Rapidox analyser is located away from extreme heat and dirt environments. Plug the unit in to a suitable supply (noting the information on the serial sticker and using the power cable supplied). Connect your gas sampling tube (6mm OD 4mm ID) to the front gas inlet connector (2). If required a second tube can be connected to the gas outlet connector (3) and vented to the outside air. If you require temperature measurement ensure that the type K thermocouple is plugged into the type K socket on the rear panel (9).

Turn the unit on using the red power switch on the front (5). At this time the internal pump will energise and you can select the required gas flow by adjusting the flow valve (4). It is recommended that the flow is adjusted to give 1 litre per min.


The LCD (1) will display the firmware version followed by the message “HEATING SENSOR”. The sensor will take approximately four minutes to come up to temperature, after which the Rapidox will begin to take measurements. The progress of the sensor heater is shown in the form of a bar graph on the LCD (1). Once at temperature the LCD display (1) will show the oxygen reading and CO₂ reading on the second line of the display. The word *ALARM* may appear to the bottom right of the LCD if the alarm system is enabled and an alarm condition applies.

Allow up to thirty minutes for the box to stabilise fully. This allows the components of the analyser to reach a stable working temperature. During this warm-up period it is common for the baseline oxygen to drift by a small amount, which may be corrected by re-calibrating.

7.1 The Rapidox Analyser - Menu System

All of the user-programmable functions are accessed via a menu system which is controlled using the front panel Keypad (2). To access the menu press the ENT button and to escape and return to the operating screen press ESC at any time. The menu system flow chart is shown below:

Rapidox 3100 Menu Flow Chart (FW v 8.2x)

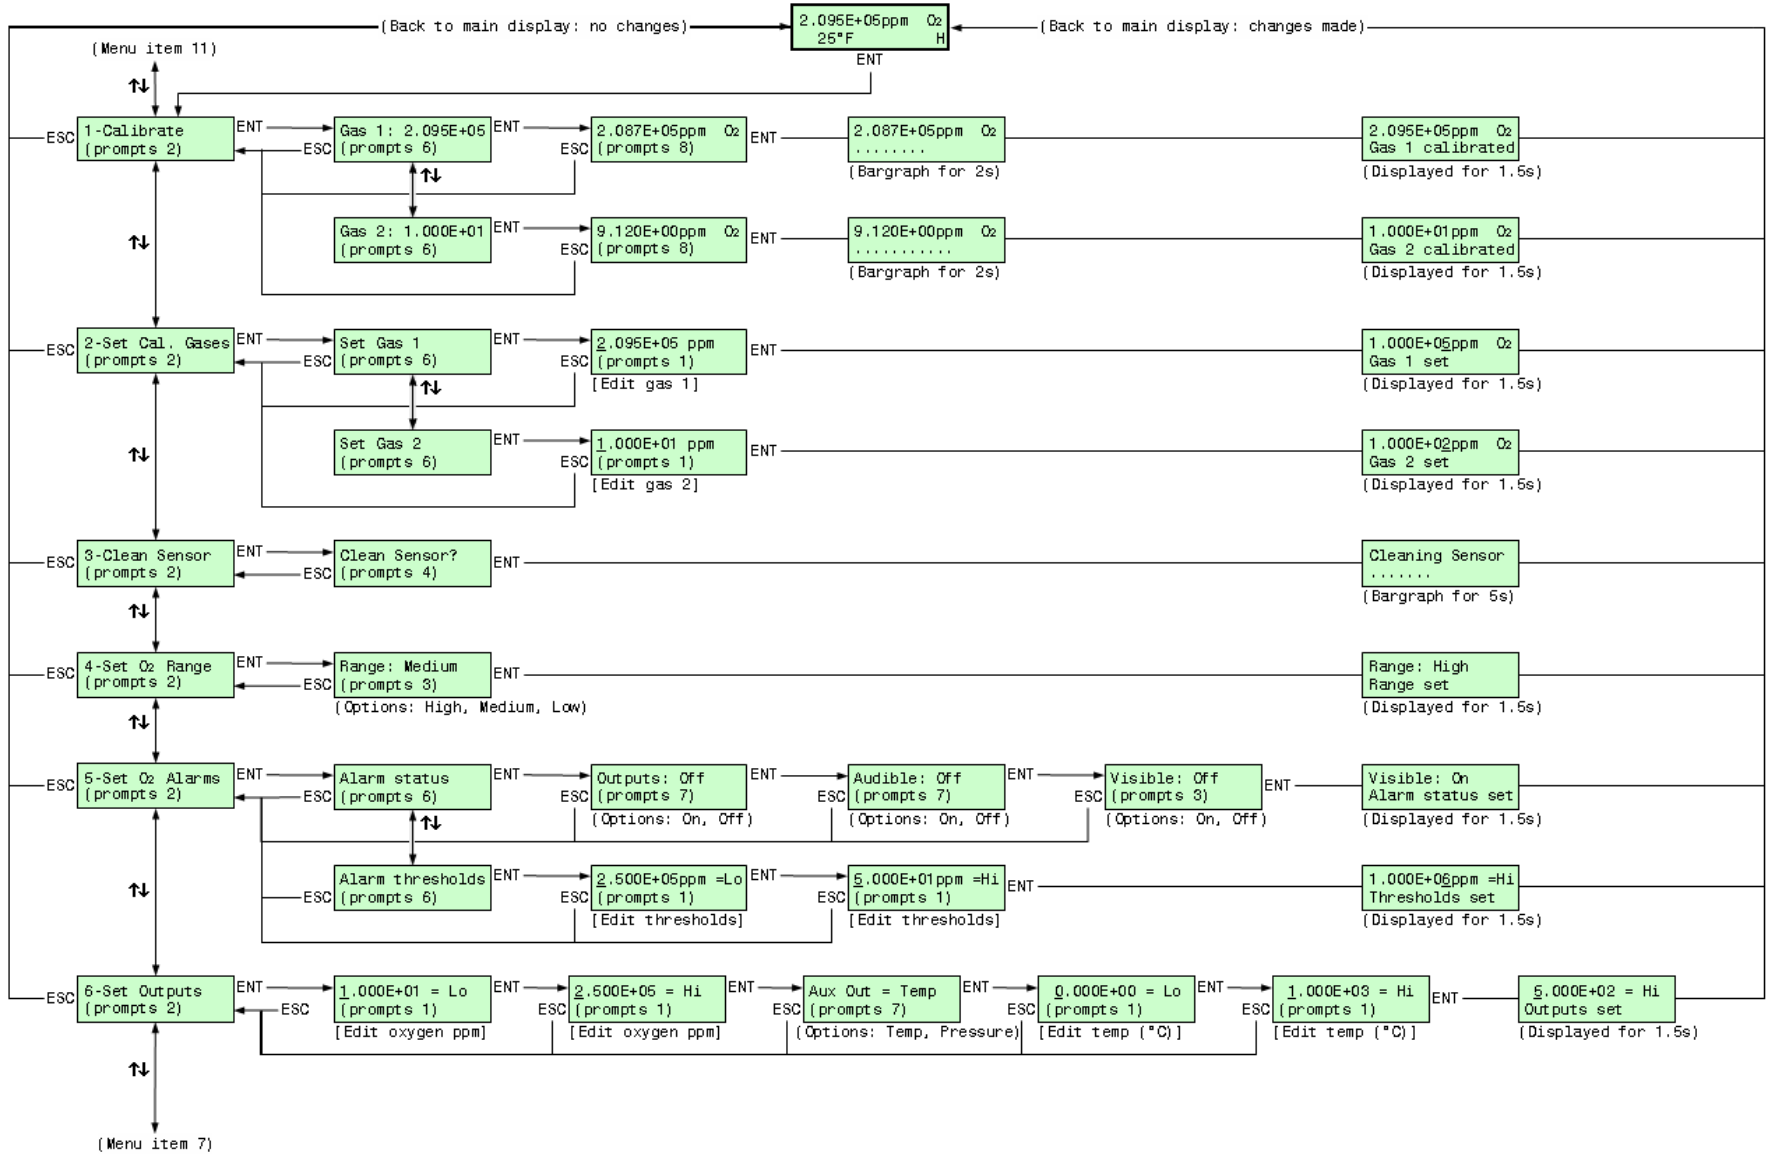

Prompts 1:
 → = Select Char.
 ↑↓ = Change
 ENT = OK
 ESC = Back

Prompts 2:
 ESC = Exit
 ↑↓ = Scroll Menu
 ENT = Next

Prompts 3:
 ↑↓ = Change
 ENT = OK
 ESC = Back

Prompts 4:
 ENT = OK
 ESC = Back


Prompts 5:
 → = Select Char.
 ENT = OK
 ESC = Back
 ↑↓ = Change

Prompts 6:
 ESC = Back
 ↑↓ = Scroll Menu
 ENT = Next

Prompts 7:
 ↑↓ = Change
 ESC = Back
 ENT = Next

Prompts 8:
 ESC = Back
 ENT for 2s = OK

Rapidox Menu Flow Chart (continued)

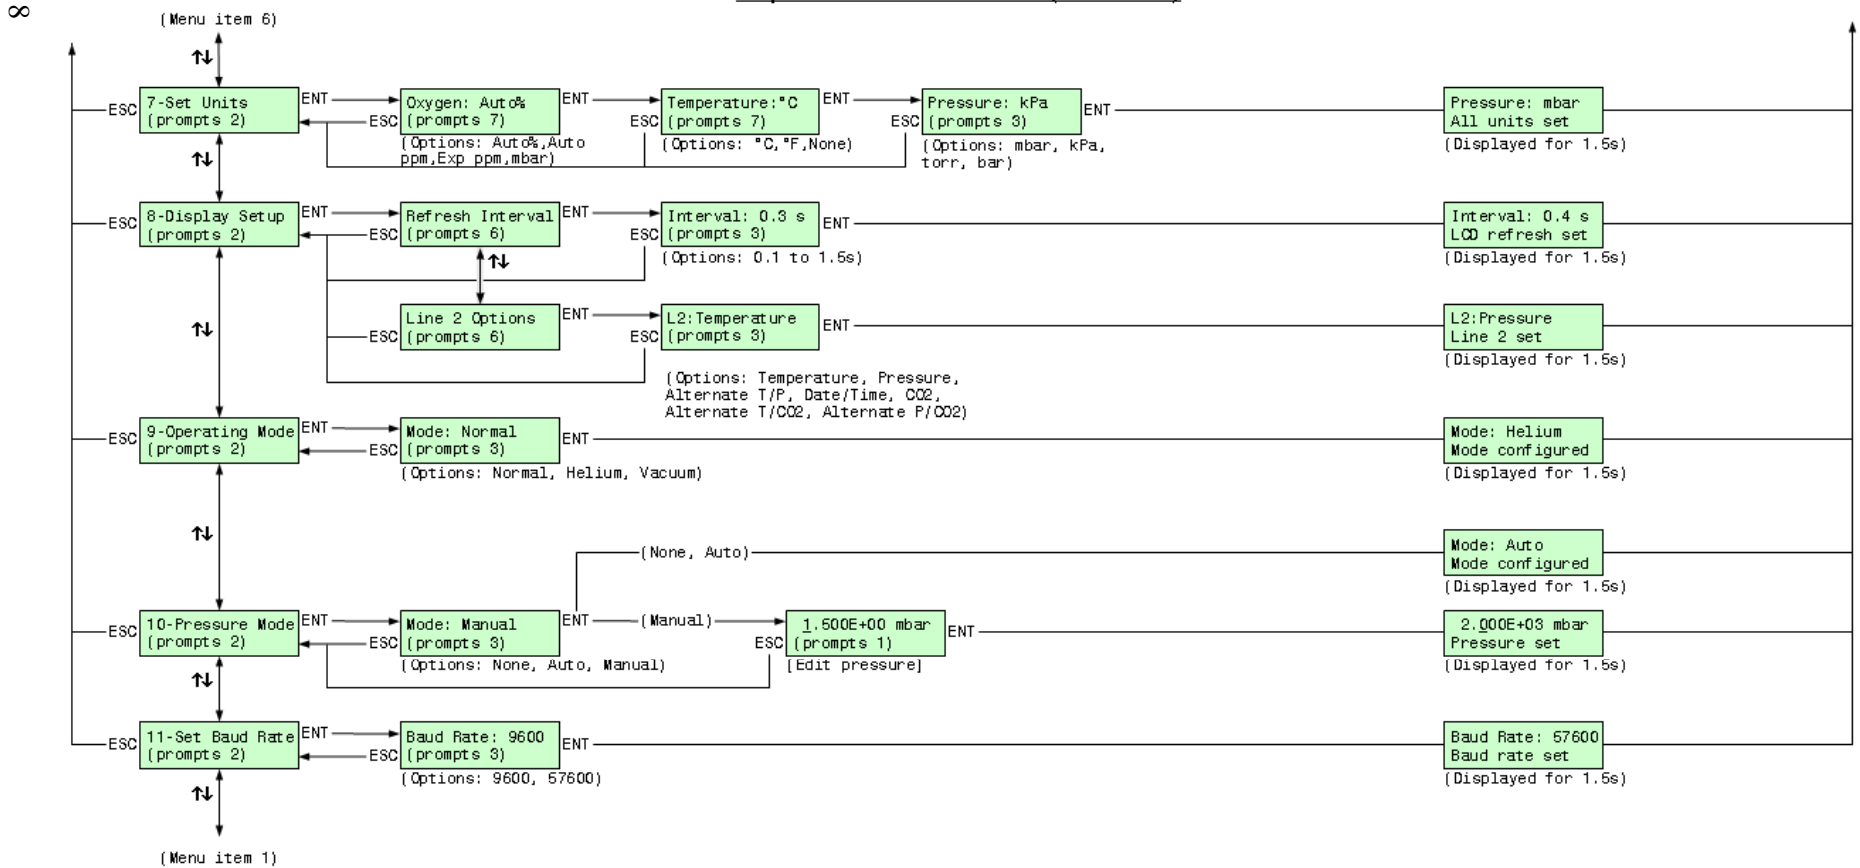

Prompts 1:
 → = Select Char.
 ENT = OK
 ESC = Back
 ↑↓ = Change

Prompts 2:
 ENT = Enter
 ESC = Exit
 ↑↓ = Scroll Menu

Prompts 3:
 ENT = OK
 ESC = Back
 ↑↓ = Change

Prompts 4:
 ENT = OK
 ESC = Back

Prompts 5:
 → = Select Char.
 ENT = OK
 ESC = Back
 ↑↓ = On/Off

Prompts 6:
 ESC = Back
 ↑↓ = Scroll Menu
 ENT = Next

Prompts 7:
 ↑↓ = Change
 ESC = Back
 ENT = Next

Prompts 8:
 ESC = Back
 ENT for 2s = OK

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

7.2 *Rapidox Calibration – Oxygen Sensor*

Once the unit is at temperature it may be necessary to calibrate the oxygen sensor². This will be necessary if you are using the sensor in a different measurement environment, to measure a different range of gases or if the gas flow changes significantly. Full calibration is a simple procedure requiring only two gases (one of which is normally air – 20.95%). The two gas values are user-selectable and can be changed by using the front keypad (6) or the communications software described in section 7.16.2, and the calibration values can be stored on file for later use.

Care must be taken to calibrate the analyser so that, whenever possible, the range of measurement lies between the two calibration points. For example, if you are working at 10ppm but have calibrated the analyser between 21% and 100% then the analyser will be inaccurate. You would need to calibrate at, say, 1ppm and 21% to be sure of good accuracy. The procedure is as follows:

- 1) Bearing in mind the points made above decide which two gases you are going to use for calibration. If you are constantly working at a particular range of compositions then it would be wise to obtain small cylinders of calibration gas with analysis certificates. You may need to programme the analyser and tell it which two gases you are using. This procedure is necessary only when you change calibration gases and is explained in section 7.3.
- 2) Press the 'ENT' button on the front panel keypad (6) to access the menu system. The calibration function is the first item on the menu list which can be scrolled using the up and down arrows. Press ENT again to enter the calibration menu. Use the UP and DOWN arrows to select either GAS 1 or GAS 2 and press ENT to proceed. The top line of the display shows the gas selected and the bottom line of the display shows the prompts. If either GAS 1 or Gas 2 are not what you require you need to reprogram the cal gases using the procedure described in section 7.3.
- 3) The sensor needs to be exposed to the first calibration gas from a cylinder (or exposed to ambient air, 20.95% if this is the calibration gas of choice). Allow several minutes to pass to flush the sensor chamber properly and make sure that the flow rate over the sensor is the same as when it is in use (1-4 litres per minute is recommended). Wait for the top line of the display (1) to become stable. To complete the calibration press and HOLD the ENT button for two seconds³. During this time you will see a bar graph progress across the lower display. The analyser will then recalibrate and display "Gas 1 recalibrated" and then return to normal run mode. The display will now correctly read the value of the first calibration gas.
- 4) To calibrate against the second calibration gas, repeat the procedure from 2 but this time press ENT followed by the UP or DOWN button to scroll

² Note that the CO₂ detector is factory calibrated and requires no further adjustment

³ Note that if the 'ENT' button is released before two seconds have elapsed, the recalibration will be aborted and the analyser will return to run mode using the existing calibration

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

- 5) through to the second screen. The second line will display the second stored calibration gas value. Flush the sensor chamber with the second calibration gas allowing several minutes for the new gas to flush through, and as before, use the same flow rate as in use (1-4 litres per minute is recommended). Wait for the display to become stable before pressing the ENT button for two seconds. The analyser will then recalibrate and display “Gas 2 recalibrated” and then return to normal run mode. The display will now correctly read the value of the first calibration gas.
- 6) The analyser is now correctly calibrated and will read accurately between these two calibration points.
- 7) If at any time, you encounter difficulties and wish to restore the machine to its factory set calibration, use the software provided and load the default settings (described in section 8.4 below). Each machine is provided with a unique file that contains the factory settings. This is located on the CD-Rom provided and is copied onto your PC during the installation process.

NB You must always perform a FULL calibration to achieve good accuracy. Only calibrate the Rapidox when in NORMAL mode and with no PRESSURE CORRECTION set (see below for details).

7.3 *Selecting the Calibration Gases*

Any two oxygen calibration gases can be used to calibrate the Rapidox 3100 although it is recommended that one is always air (20.95%). You can reprogram the two calibration gases to suite your needs via the menu (6) on the front panel or by using the software provided (see section 8.5.2). Press ENT to access the menu and scroll down to option 2 “Set Cal. Gases”. Press ENT to proceed. Use the UP and DOWN arrows to select cal gas 1 or cal gas 2. Press ENT to edit the value. On the edit screen you can use the RIGHT arrow to move the blinking cursor across to the character you wish to change⁴. Use the UP & DOWN keys to change the value. You can also change the sign of the exponent in the same way. Note that for ease of editing the cal gases are written in ppm Exponent format so air (20.95%) would read 2.095E+05ppm. When you have finished editing the value press ENT to store it in memory. Now repeat the operation for the second cal gas. These values will remain in memory until you re-edit them in the future.

7.4 *Cleaning the Sensor*

You can clean the oxygen sensor at any time by pressing ENT on the keypad (6) and scrolling down to option 3 “Clean Sensor” or using the software described in section 8.7. Press the ENT button to proceed. The screen displays “Clean Sensor?” Press ENT again and the cleaning will take place. The procedure takes approximately five seconds and the LCD display shows the progress of the operation. Once finished the analyser will take a moment to re-stabilise. The sensor is cleaned each time the unit

⁴ Note that you can not go back to edit a previous value. Instead keep pressing the RIGHT button and the cursor will wrap around back to the beginning. Alternatively press ESC to start again.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

is switched on prior to operation. If you are operating in gases with large amounts of soot, there is a risk that the sensor surfaces will become contaminated with particulates, which will impair performance if allowed to build up. The cleaning operation pumps oxygen through the zirconia tube, which burns the particulates away from the sensor surface.

7.5 *Oxygen Sensor Range*⁵

The Rapidox 3100 is fitted with three ranges of oxygen which can be programmed using the Keypad (6) or the software provided (section 8.5.2). Always select the most appropriate range to work with to achieve maximum resolution from the analyser. The three ranges are labelled LOW, MEDIUM & HIGH⁶.

High	from 0.1% to 100% oxygen
Medium	from 0.001% to 100% oxygen
Low	from 10E-20ppm to 100% oxygen

The range currently in use is displayed in the bottom right hand corner of the LCD display (1) by the character L, M or H. To change the range select option 4 “Select O₂ Range” and press ENT. Use the UP & DOWN arrows to select the required range and press ENT to finish.

7.6 *Alarms*

The Rapidox is fitted with fully programmable oxygen alarms. There are two independent alarm circuits for low and high oxygen conditions. These are relay circuits which are open if there is no alarm and closed when an alarm condition occurs⁷. You have the option of enabling the alarm circuits, enabling an audible buzzer and enabling a visual warning on the screen.

The alarm set points can be programmed by the user via the keypad (6) on the front panel or using the software provided (section 8.5.2). To change the alarm set point scroll down the menu to no. 5 “Set O₂ Alarms” and press ENT. Now use the UP & DOWN arrows to select “Alarm Thresholds” and press ENT. The next screen shows the alarm low setting which can be modified in the same way as described in 7.3 for the cal gases. Press ENT when finished and repeat for the high alarm setting. Press ENT to finish and return to normal operation.

To modify the alarm options select menu no. 5 again and use the UP & DOWN arrows to select “Alarm Status”. Here you are given the option to enable or disable the outputs on the rear, enable or disable the audible buzzer & enable or disable the

⁵ The CO₂ sensor range is fixed on the card and must be specified at the time of ordering. The ranges available are 0-5%, 0-10%, & 0-20% CO₂

⁶ Note that if you operate the machine below the minimum value of a particular range the display will ‘bottom out’ and you need to select a lower range to continue measuring.

⁷ Note that the alarm circuit relays are accessed via the terminal block on the rear panel and are clearly labelled. The relay circuit is rated at 24V 0.5amps maximum.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

warning on the front screen. Use the UP & DOWN arrows to select each option and ENT to proceed and finish. When the alarm is activated the warning buzzer will sound and the front display will flash the word ALARM in the lower right hand corner.

7.7 *Analogue Outputs*

The Rapidox 3100 analyser provides various analogue outputs. The standard industrial analogue outputs (0-5V and 4-20mA) for both oxygen and CO₂, temperature or pressure, are accessible via the terminal block (7) on the rear panel⁸. In the case of oxygen, the outputs are factory set to provide a linear response in the range 0-25% that will cover most applications. However because of the large range of oxygen covered by the analyser, the lower and upper values are fully user-programmable using the keypad (6) or the software provided (section 8.5.2).

The auxiliary outputs can be set to either 'CO₂', 'Temperature' or 'Pressure'. The second option will output the value read from the thermocouple when attached. The third option will output the value read from the internal pressure sensor⁹.

To modify the oxygen analogue output range scroll down the menu to no.6 "Set Outputs" and press ENT. You can now edit the lower and upper values in exactly the same manner as described in 7.3 for setting the cal gas values. Once programmed the new values remain in the memory until they are edited again in the future.

To select and modify the auxiliary outputs scroll down to menu option 6 "Set Outputs" and press ENT three times. Use the up and down arrow buttons to choose between "CO₂" "Temperature" and "Pressure" and press ENT.

If "CO₂" is selected then chose the range of the sensor installed in your machine.

If "Temperature" is selected then you can change the low and high settings using the same procedure described in section 7.3. The range is set between 0°C and 1000°C

If "Pressure" is selected then the permissible range of the internally located pressure sensor is -1000 to +1000 mbar

7.8 *Setting the Display Units*

The notation used by the display (1) is fully programmable to suit your needs using the keypad (6) or the software provided. The following options are available to you:

Oxygen: The oxygen reading can be displayed in percent (e.g. 20.95%), ppm (e.g. 209500ppm) or scientific (e.g. 2.095E+05ppm). There is also an option to display

⁸ Note that the ranges of the 0-5V and 4-20mA are tied together so changing one alters the other.

⁹ Note that the fault signal for the auxiliary outputs is 0V / 1mA. If the thermocouple is disconnected then the output will drop to these values to warn the user of a problem.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

the oxygen reading in terms of a pressure in mbar. If Auto Percent is selected the Rapidox will display oxygen as a percentage down to 0.1% and ppm below this value. At values less than 1ppm the display switches to scientific notation for the remainder of the range.

Temperature: The thermocouple reading can be displayed in Celsius (°C) or Fahrenheit (°F).

Pressure: The internal pressure sensor reading can be displayed as mbar, bar, torr or kPa.

To program these options scroll down to menu no. 7 “Set Units” and press ENT. Use the ENT key to progress through the list and the UP & DOWN keys to select the required units. Once selected press ENT to store and return to run mode.

7.9 Setting the Display Options

The user can select the LCD refresh rate and the format of the line 2 display using the keypad or the software provided. Scroll down the menu to option no. 8 “Set up Display” and press ENT. Use the UP & DOWN arrows to select either the LCD refresh rate or Line 2 Options:

LCD Refresh Interval: The frequency of the display update can be selected from 0.1 to 1.5 seconds. The current setting can be edited using the same method as described in 7.3 for modifying the cal gases. Once edited press ENT to store and return to normal operating mode.

Line 2 Options: The information displayed on line 2 of the LCD can be chosen by the user. The options are Temperature (displayed 0-1000°C or °F), Pressure (displayed in mbar, bar, torr or kPa), Alternate T/P (both temperature and pressure are displayed alternately), the date and time (displayed dd/mm/yy HH:mm:ss), CO₂ (displayed in %), Alternate T/CO₂ or Alternate P/CO₂. Use the UP & DOWN arrows to select the display required and press ENT to store and return to normal operating mode. The default is CO₂ on a Rapidox fitted with a CO₂ detector.

7.10 Operating Mode

The Rapidox 3100 has some additional features to enable the unit to work in helium gas mixtures or in partial vacuum systems as described below. These can be programmed using the keypad on the front panel or the software provided.

Helium: Helium presents a challenge to the analyser because of the high thermal conductivity of the gas. In normal mode the heater setting is not powerful enough to cope with the cooling effects of helium, so the Helium Mode should be selected. This allows the Rapidox 3100 to operate with helium flowing over the sensor. The analyser will give good readings in helium but the following points should be noted:

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

1. The sensor response time is reduced compared to oxygen operation
2. The sensor will require a new calibration to operate correctly in helium (i.e. using helium calibration gases)
3. The sensor may overshoot when changing gas compositions rapidly as it needs more time to cool and heat up.
4. The Rapidox will not function properly in other gases (e.g. air) whilst in helium mode. Only helium mixtures should be used.

When the helium mode is selected it is normal for the Rapidox 3100 to go back into heating mode until the new heater setting is reached and settles down. The same happens when returning to 'normal' mode of operation. When helium mode is selected the symbol "He" appears on the second line of the display to remind you.

Vacuum: This option allows the user to operate the Rapidox 3100 as though it were a vacuum gauge. The sensor will respond to changes in vacuum in the same way as changes in oxygen. So for example if the vacuum is increased to 500mbar then the sensor will change from 20.95% to 10.5% as there is a linear relationship between vacuum and oxygen partial pressure.

The sensor will respond well in partial vacuums but the analyser is not designed to run under high vacuum (i.e. more than 1000 mbar below atmospheric).

To programme the mode of operation scroll down the menu to no. 9 "Operating Mode" and press ENT. Use the UP & DOWN arrows to select the required mode: Normal (factory default for oxygen measuring), Helium (for use in helium gases) & Vacuum (for use in vacuum systems). Press ENT to store the mode into memory and proceed. The LCD display (1) will show the text "He" or "Vacuum" to indicate that a special mode is in operation.

7.11 *Internal Pressure Sensor*

The Rapidox 3100 is fitted with an internal pressure sensor which monitors small changes in pressure and vacuum inside the sensor head¹⁰. The pressure will normally be zero mbar under normal operation but if the unit is being fed by a gas cylinder or connected to an apparatus under partial vacuum then the pressure will change and this will have a direct effect on the oxygen partial pressure and the sensor reading. You have the option of displaying the pressure reading on the LCD display (1). Select no. 8 "Set Up Display" and press ENT. Select "Line 2 Options" using the UP & DOWN arrows and press ENT. You can set the display to read Temperature, Pressure, Alternate T/P or the Date & Time. Select Pressure and press ENT. The display will now show the pressure reading from the internal sensor. If you want to view different units select no. 7 "Set Units" from the menu and press ENT three times to reach the pressure screen. Use the UP & DOWN arrows to select

¹⁰ The pressure sensor can be used as a totally independent sensor or can be used to correct for oxygen partial pressure measured by the oxygen sensor. This is explained in section 7.12. The scale of the pressure sensor fitted is +/- 1000 mbar.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

mbar, bar, torr or kPa and press ENT. The display will now show the pressure in the selected units.

7.12 Pressure Mode

The user has the option of using the reading from the internal pressure sensor to automatically correct for changes in gas pressure and hence oxygen pressure. A manual pressure correction value can also be used. To access this function scroll down to menu option 10. "Pressure Mode" and press ENT. The desired mode can then be selected using the UP & DOWN arrows and pressing ENT to store and proceed. The three modes available are:

Normal: If this mode is selected then there is no pressure correction performed on the oxygen reading. The pressure and oxygen sensor act independently. If the sensor is working in air (20.95%) and the pressure is doubled to 1000 mbar then the reading will also double to 41.9%. This is the correct oxygen partial pressure in air at 2 bar since there is a simple linear relationship between pressure and concentration.

Auto: This is the factory default setting. If the Auto mode is selected then the Rapidox 3100 takes then reading from the internal pressure sensor and corrects the oxygen partial pressure to maintain a concentration reading. If the sensor is working in air (20.95%) and the pressure suddenly jumped to, for example, 500 mbar above atmospheric, the oxygen reading would remain at 20.95% because the sensor has been corrected for the pressure change. This allows users who are working with fluctuating input pressures to maintain a 'meaningful' reading of oxygen concentration that will only be affected by changes in gas composition and not gas pressure.

Manual: The user can ignore the internal pressure sensor and manually enter a pressure value to perform the correction¹¹. If, for example, the user wants to measure air at 500 mbar pressure above atmospheric then normally the analyser would display $1.5 \times 20.95 = 31.43\% \text{ O}_2$. However the user always works at 500 mbar pressure and wants to display corrected oxygen concentration. So by manually entering 0.5 as the pressure the reading will once again display 20.95%

7.13 Setting the Baud Rate

If you are using the software for data logging you can chose the communications speed (Baud Rate) by scrolling down the menu to no. 11 "Baud Rate" and using the UP & DOWN arrows to select either 9600 or 57,000. Press ENT button again to store and return to normal operation. The default factory setting is 57000. However if you are using an older PC you can decrease this to 9,600 to improve the reliability of the software and data communications.

¹¹ Important: take care when using this last function. If you stop working under pressure or the pressure is changed then the Rapidox 3100 will display incorrect results until the manual setting is either reset or changed to the correct value.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

7.14 Load Defaults

If you make a mistake programming the Rapidox it is possible to restore the machine back to its factory settings by loading the unique default configuration that is supplied on your software CD-rom. The default set-up can only be accessed using the software provided. Please see section 8.4 for further details.

7.15 Type K Thermocouple

The type K thermocouple (supplied) is connected via the socket on the rear panel (8). When fitted correctly the LCD display (1) will show the temperature in Celsius (or Fahrenheit if selected). If this is not the case then you need to select the display option in the menu system as described in 7.9. Press ENT and scroll down to no. 8 "Set Up Display". Press ENT to access and then press the DOWN arrow to select "Line 2 Options". Press ENT to access this menu. Select "Temperature" and press ENT to confirm. The display should now read the temperature. If you want to display the temperature in Fahrenheit instead of Celsius select option 7 "Set Units" on the menu and press ENT again to access "Temperature". Select the desired units (or NONE to disable) with the UP & DOWN arrows and press ENT. The display will now update.

The thermocouple is an independent measurement from the oxygen sensor, and it is not necessary to have it connected for oxygen measurements. The thermocouple can be positioned anywhere you desire but typically it is placed in close proximity to the oxygen sensor so the measurement gas temperature may be recorded. The type K thermocouple measurement displays 0 to 1000°C and is accurate +/- 1%.

7.16 RS232 / RS485 Port

It is possible to factory set the data communications port to either RS232 or RS485. Once configured at the factory it is not possible to change unless the unit is returned to Cambridge Sensotec Ltd.

Data from the Rapidox is sent on demand to the 9-way 'D' type socket RS232 port (8) on the rear panel and can be read using a simple terminal programme such as 'HyperTerminal' in Windows, or with the user's own custom software. Alternatively a simple and convenient data-logger programme is included with the supplied software and is described in section 9 below.

7.16.1 RS232 Protocol

The RS232 port will output data on demand at a maximum rate of approximately 4 readings per second. To request data, send the single character command ASCII 'D'. The analyser should reply with a comma separated string of which the first character will always be 'd' in response to the data request command, and the last two characters will be ASCII codes 13 and 10 (i.e., carriage return CR and line feed LF).

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

The comma separated data fields in the output string are as follows: oxygen concentration (pressure corrected if enabled) in ppm exponent format, sensor emf in mV, pressure (or "0" if no pressure sensor) in bar, temperature (or "*" if no thermocouple or fault) in current units, CO₂ in percent exponent format, time (in "hh:mm:ss" format), date (in "dd/mm/yy" format), oxygen range ("L", "M" or "H"), operating mode (nothing, "He" or "Vac"), and finally "ALARM" if an alarm is active. There is no comma between the initial 'd' and the oxygen reading. Note that the output string always uses the period '.' as a decimal separator, and that this is recognised by the supplied data-logging software whatever the regional settings of the PC.

If the character returned by the Rapidox in response to 'D' is '?' then it has not recognised the command, which should be sent again. If the 'D' command is sent while the analyser is not in normal run mode, it will reply with '!' followed by a message indicating why it is busy, ending with CR/LF. Wait for the analyser to enter run mode or if it's in local setup mode via the front panel, either complete the setup or exit the menu before continuing. The analyser is in normal run mode when it is not in the local setup menu and is displaying oxygen continuously on the LCD.

The RS232 port settings are 8 data bits, no parity, 1 stop bit. There is no flow control. The baud rate can be set to either 9600 or 57600 and is selected using option 11 on the menu ("Baud Rate") as described in 7.16. The analyser's connections to the 9-way socket are: Tx (data out) = pin 2, Rx (data in) = pin 3, Signal Ground = pin 5; all other pins are unused.

When using RS232 make sure to use the data cable supplied, or an equivalent. This is a 9-way male to female straight through connector (i.e. pin1 to pin 1, pin 2 to pin 2 and so on). No other type of cable will work. If you wish to use a custom cable, you only need three wires, between connector pins 2, 3 and 5, as noted above.

7.16.2 RS485 Protocol

Please contact Cambridge Sensotec for further information on this new feature.

8. Rapidox Software Instructions

8.1 *Software Installation*

It is possible to program a range of variables to the Rapidox using an RS232 (or RS485 if configured) link with a PC running MS-Windows (all versions) and the supplied Rapidox software. The software is installed automatically by inserting the Rapidox CD into the CD-ROM drive. If auto-installation does not start then you can click the Windows START button and select RUN. Type X:\setup.exe where X is the drive letter of your CD. Alternatively access the CD from Windows Explorer or the 'My Computer' icon on your desktop, and double-click on the 'Setup.exe' programme. Follow the on-screen instructions to install the programme onto the hard drive. Once installed you can access the programme by clicking START - PROGRAMS – Rapidox Software¹².

8.2 *Getting Started*

Make sure that the Rapidox is connected to a free serial port on the rear of your computer. These will nearly always be COM1 or COM2 but the software will scan through the ports until it finds the Rapidox. The analyser must be switched on for this to succeed and while you are communicating with it. You can programme the variables without a sensor attached, but to monitor the Rapidox properly, the sensor needs to be connected and at operating temperature. On start up the software will locate the Rapidox and display the following page¹³:

¹² The software has been tested successfully on most language machines including Chinese & Japanese.

¹³ The values displayed in the columns of boxes above the 'Read' and 'Write' buttons may differ from those shown.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

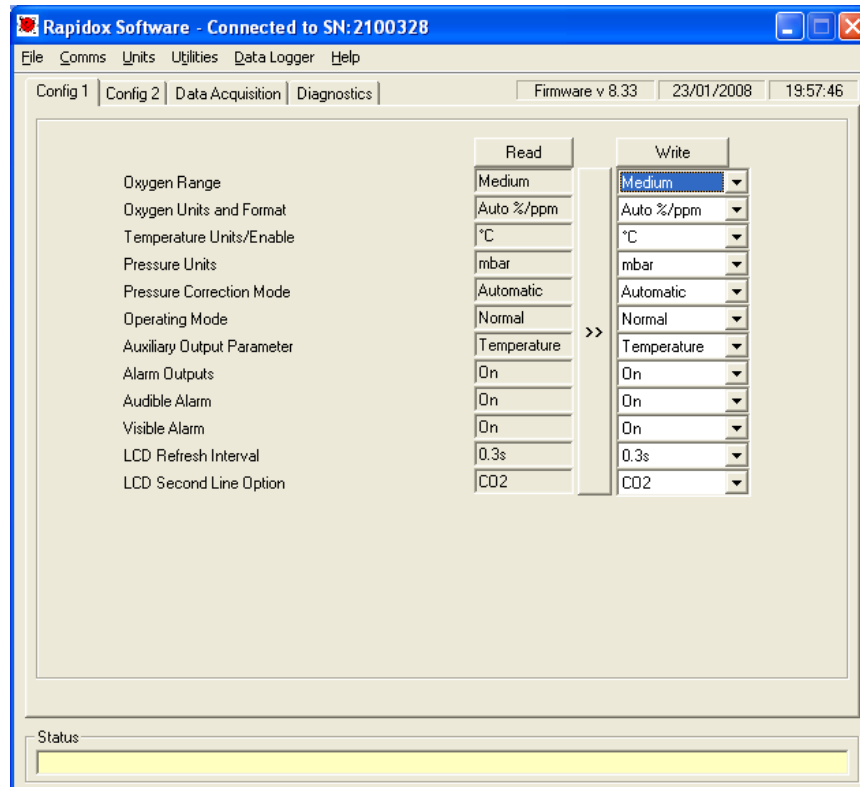


Figure 3: Rapidox configuration page

The yellow status box at the bottom will display confirmation that the Rapidox was found and the result of the last action, or any error messages if there is a problem with communication. If you experience problems check that your serial cable¹⁴ (supplied) is correctly fitted to a valid serial port. Also check the status of your COM port settings in Device Manager accessed by clicking START – Settings - Control Panel.

8.3 On-Screen Help

You can access the on-screen help facility at any time by clicking on the help menu on the menu bar and select the 'Help' option or press F1.

8.4 Configuration Page

The configuration page is split into two and you can toggle by clicking on the folder tabs labelled "config 1" and "config 2" page allows the user to reprogram an array of variables used by the Rapidox. Once written to the Rapidox, the new variables remain permanent until overwritten.

¹⁴ There are several types of serial cable available. You must use a cable as supplied where there are straight through connections, i.e., pin 2 to pin 2, pin 3 to pin 3 and pin 5 to pin 5. Other cable formats will not work.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

To read the current configuration stored in your Rapidox select 'Read Analyser Configuration' from the file menu. Note that the edit boxes on the RHS will turn red if the value is different to that just read and a red asterisk will appear next to the 'Write' button to warn you that a change has been made. The left-hand set of grey text fields ('read fields') will be updated with the current configuration data. To save this information (e.g., if several people share the same instrument) press the long copy button to transfer the data into the edit boxes, select 'Save Configuration as' from the file menu and choose a filename. This data set can be subsequently be reloaded at any time by selecting 'Load Configuration File' button and selecting the directory where the configuration files have been stored.

If at any time you wish to restore the machine to its factory default settings select 'Default Configuration' from the file menu to load these values. The software will search for a unique rxc file that is loaded onto the PC during the software installation. The filename is 2100***.rxc where *** is the last three digits of the serial number located on the rear of the machine. This file is also located on the CD-Rom that came with the machine. Normally this file is located in the main Rapidox directory but if the software can not locate it then it will ask you for the serial number to help it search. With the correct rxc file loaded simply press COPY to transfer the defaults into the edit boxes and then select WRITE to load them back into the Rapidox.

The right-hand set of white editable text fields ('write fields') is used to enter new values to be programmed into the Rapidox. The values in these fields can either be entered manually, or copied across from the 'read fields' by clicking the vertical 'Copy' button, and then edited as required¹⁵. Alternatively, you can load saved configuration data by selecting 'Load Configuration' from the file menu and selecting the required file. In order to programme the analyser select 'Write configuration to the analyser' from the file menu.

8.5 Reconfiguring the Analyser

The on-screen edit boxes contain variables that can be reprogrammed into the Rapidox in exactly the same manner as using the front Keypad. For a full description please refer to the relevant section in this manual.

The user can choose whether to use ppm or percent notation to edit the text boxes by selecting the UNITS menu and clicking on percent or ppm. To access a field, either click inside it or use the TAB key to scroll through them. The field parameters are as follows:

¹⁵ Note that when you click on the copy button both pages are updated at the same time and there is no need to repeat the action when you toggle to the other page.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

8.5.1 Config 1 Screen

- 1) **Oxygen Range:** See section 7.5 for a full description. Use the drop down box to select LOW, MEDIUM or HIGH. The default setting is Medium.
- 2) **Oxygen Units & Format:** See Section 7.8 for a full description. Use the drop down box to select PPM EXPONENTIAL, PPM MIXED, AUTO%/PPM or PRESSURE. The default setting is AUTO%/PPM.
- 3) **Temperature Units/Enable:** See sections 7.8 and 7.15 for a full description. Use the drop down menu to select °C, °F or NONE. If NONE is selected then the temperature display is completely disabled. The default is °C.
- 4) **Pressure Units:** See sections 7.8 and 7.11 for a full description. Use the drop down menu to select MBAR, TORR or KPa as the unit for pressure measurement. The default setting is MBAR.
- 5) **Pressure Correction Mode:** See section 7.12 for a full description. Use the drop down menu to select NONE, AUTOMATIC or MANUAL. The default setting is AUTO.
- 6) **Operating Mode:** See section 7.10 for a full description. Use the drop down menu to select NORMAL, HELIUM or VACUUM. The default setting is NORMAL.
- 7) **Auxiliary Output Parameter:** This function allows the user to choose whether the Auxiliary output terminals on the rear panel (6) are for use with the thermocouple (7) or the optional pressure sensor (4). Use the drop down menu to select CO₂, TEMPERATURE or PRESSURE. The default setting is CO₂.
- 8) **Alarm Outputs:** See section 7.7 for a full description. Use the drop down menu to select OFF or ON. When set to ON the alarm circuits on the rear are activated. The default setting is ON.
- 9) **Audible Alarm:** See section 7.6 for a full description. Use the drop down menu to select OFF or ON. When set to ON the buzzer will sound when an alarm is activated. The default setting is ON.
- 10) **Visible Alarm:** See section 7.6 for a full description. Use the drop down menu to select OFF or ON. When set to ON the front display will show the word ALARM (flashing) when an alarm is activated. The default setting is ON.
- 11) **LCD Refresh interval:** Use the drop down menu to select a refresh rate for the LCD (min 0.1, max 1.5 sec). The default is 0.3 seconds.
- 12) **LCD Second Line Option:** See section 7.9 for a full description. Use the drop down menu to select TEMPERATURE, PRESSURE, ALTERNATE T/P,

DATE/TIME, CO₂, ALTERNATE T/CO₂, ALTERNATE P/CO₂. The default setting is CO₂.

8.5.2 Config 2 Screen

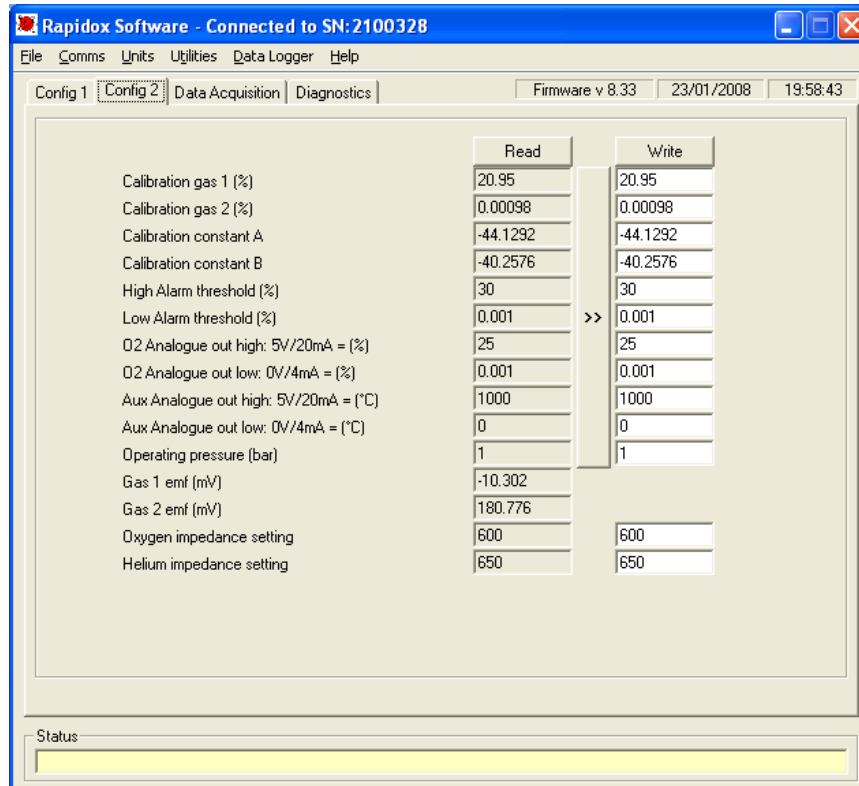


Figure 4: Configuration 2 page

- 13) **Calibration Gas 1:** Use this box to enter a new value for the first cal gas. The value can be entered either in % or ppm depending on the units selected. The default is %. Enter a value such as 10.1 for 10.1%¹⁶. The default value for cal gas 1 is 20.95%
- 14) **Calibration Gas 2:** Use this box to enter a new value for the second cal gas. The value can be entered either in % or ppm depending on the units selected. The default is %. Enter a value such as 0.1 for 0.1%. The default value for cal gas 2 is 0.001% (10ppm).
- 15) **Calibration Constant A & B:** These boxes contain the calibration constants that the Rapidox calculates automatically when you perform a

¹⁶ Note that software is 'regionally aware' and will therefore accept and display data using the decimal separator that is set in the PC's Regional Settings in the Control Panel. For example, in the UK or US, you might enter the value 2.5 - in continental Europe this would normally be entered as 2,5 assuming the PC's Regional Settings have been set up to use ',' as the decimal separator. The software also works with non-English versions of Windows including Chinese.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

calibration. You will see that they change each time you perform a new calibration. It is possible to manually edit these but this should only be attempted after consulting with Cambridge Sensotec. Normally they are just provided for information and should be left untouched. The default settings are A= -46.482 and B= -38.845. Note that the values are always negative as this follows the convention of the Nernst equation.

- 16) **High & Low Alarm Thresholds:** Use these two boxes to enter new values for the alarm trigger points. The alarm High value must always be greater than the alarm low value. The value can be entered either in % or ppm depending on the units selected. The default is %. Enter a value such as 10.1 for 10.1%. The default values are 25% for Alarm High and 0.001% for Alarm Low.
- 17) **O₂ Analogue Output (0V/4mA & 5V/20mA):** Use these two boxes to set the High and Low oxygen values for the analogue outputs (6) on the rear panel. For example if you want 4mA to represent 1% and 20mA to represent 21% then enter these two values into the appropriate boxes. The value can be entered either in % or ppm depending on the units selected. The default is %. The default values are 25% for the high setting and 0.001% for the low setting.
- 18) **Operating Pressure:** Use this box if you want manual pressure correction of the oxygen reading. Enter a value in bar (e.g. 1.0). In this case air (20.95%) will give a reading of 41.9% (true oxygen partial pressure) at 1 bar but if the manual correction is set to 2.0 then the reading will be corrected back to 20.95% which is the true concentration. The default value is 0 (no correction).
- 19) **Gas 1 & Gas 2 emf (mV):** These values are for information purposes only and cannot be adjusted. They represent the voltage that the Rapidox measured on the sensor at the point of calibration. These values are used in the calculation of the A & B values derived from the Nernst equation. As a guide the emf in air is around -8mV and the value at 10ppm is around +190mV. Exact values depend entirely on the individual sensor.
- 20) **Oxygen and helium impedance setting:** These values are for information purposes only and can not be adjusted. They control the temperature of the heater for the two modes of operation by setting the impedance of the zirconia cell to a pre-determined value.

Once you have finished editing the parameters, select 'Write Configuration to Analyser' from the file menu and the new data set will be written to the Rapidox. The Rapidox is reprogrammed using the new configuration. The software then reads the new settings back from the Rapidox and displays them in the boxes on the left-hand side confirming that the configuration was successful. When you have finished programming the analyser for new calibration gases you must recalibrate the instrument to benefit from the changes.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

8.6 On-Screen LCD

It is possible to display an LCD emulator on the desktop of your PC. This reproduces exactly the display on the Rapidox unit and is convenient if you are some distance away from the machine. To activate the LCD select the utilities menu and select the LCD on option. This will display a small window showing the LCD that can be positioned independently anywhere on the desktop.

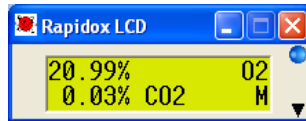


Figure 5: On-screen LCD

The blue LED indicator will flash to show that the display is updating.

8.7 Remote Calibrating and Cleaning

With the on-screen LCD display active it is possible to remotely calibrate the oxygen sensor and clean the sensor. Click on the down arrow icon in the bottom right-hand corner of the LCD display to expand the window:

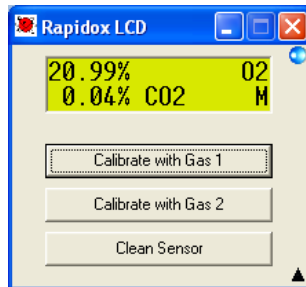


Figure 6: Remote calibration and clean function

Use the three buttons to calibrate or clean the sensor directly from the PC. Note that you will receive a prompt asking you if you wish to proceed before the calibration actually takes place.

8.8 Setting Analyser Date and Time

The current date and time of your PC are displayed on the configuration screen and can be loaded into the Rapidox by selecting the Utilities menu and clicking the 'Set date and time' option. This information is used in the RS232 data string for data logging purposes. Make sure that your PC clock is set correctly before using this function, as you cannot edit the date and time shown by the Rapidox software. The date and time formats displayed are those set in the PC's Regional Settings.

9. Rapidox Data-Logging Software

9.1 Introduction

The Rapidox software includes a full data logging facility. Data can be saved to a file automatically at regular intervals and the format is compatible with modern spreadsheet programmes such as MS-Excel. A live-time graphing facility is also included which has many powerful features. Note that the data logging facility will only function if the analyser is in NORMAL run mode.

9.2 Setting up the Data Logger

Click on the tab labelled 'Data Acquisition' to display the following page:

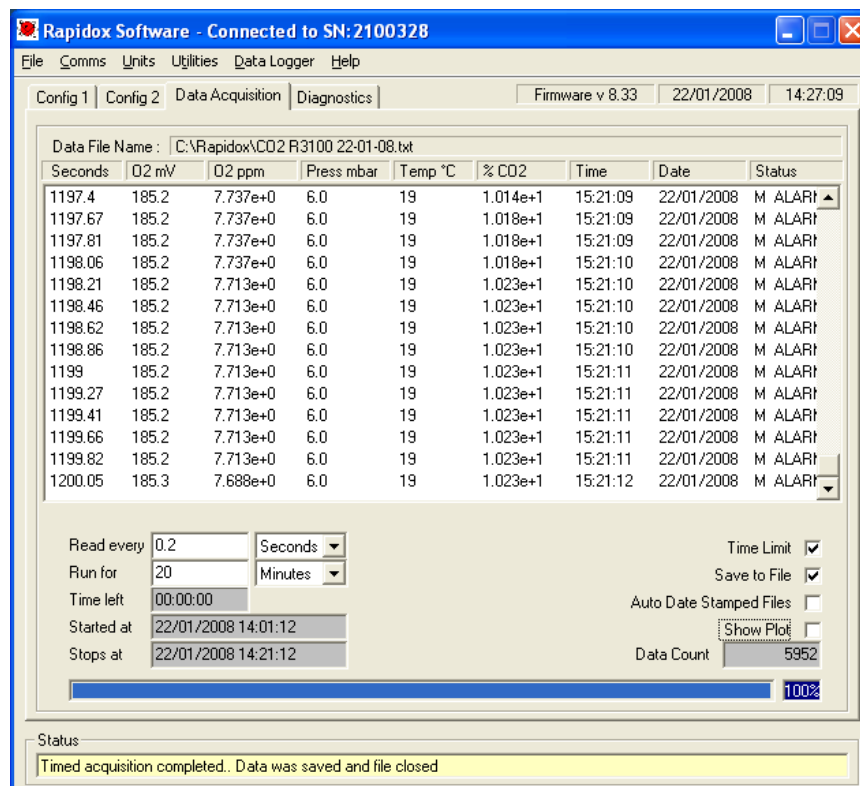


Figure 7: Data Logging page

During logging, data from the analyser is shown in the central area of this page. The data is displayed in the following columns: time (in seconds), the raw signal from the sensor (in mV), the oxygen value (in ppm scientific notation), pressure in

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

mbar, the type K thermocouple reading (in Celsius), CO₂ sensor value (in percent scientific notation), the time (in regional format), the date (in regional format), and status (displays the range setting or the word ALARM if the alarm is activated).

To start data logging select the frequency of measurement by entering a time and selecting a unit from the drop down list. For example if you wish to log data once every minute type 1 in the box and select 'Mins' from the drop down menu.

You can open the notes window at any time by selecting NOTES from the 'Data Logger' drop down menu. A small text box appears in which you can type a text message. This note is then saved as a header in the data file set and can be viewed along with the data.

You can either choose to have data logged continuously until 'Stop' is selected from the Data Logger menu, or you can choose to set a time limit for data logging by checking the box labelled 'Time Limit', setting the duration in the 'Run For' box and selecting units with the drop down list. For example if you wish to log data for thirty minutes type '30' in the box and select 'Mins' from the drop down list.

9.3 *Running the Data Logger*

If you wish to save the data into a file for later use, check the 'Save to File' box before selecting 'Run' from the Data Logger menu. You will be prompted for a file name and location before data logging commences. The file and path information will appear in the box at the top of the page labelled 'Data File Name'. If you forget to select file saving before starting a run, you will nevertheless be prompted at the end as to whether you wish to save the run data.

The blue progress bar displays the state of completion of the run, and the blue box to the right of it the same information as a percentage. You can stop the run at any time by selecting 'Stop' from the Data Logger menu. The yellow Status bar at the bottom of the page gives information about the data logging operation.

Once data logging is complete you may open the text format data file using any compatible spreadsheet programme such as MS Excel, and use the data to generate plots and reports.

You can pause the data logger at any time by selecting 'datalogger' and 'pause'. Repeat to continue logging from where you left off, noting that the clock keeps ticking during the pause period.

9.4 *Auto Date Stamped Files*

If you are planning to run the data logger for extended periods of time then you should consider checking the 'Auto date stamped file' option. This feature will save the data at midnight for the previous twenty four hours and so on until the data-logging is complete OR the user interrupts. The data file is stored with a date suffix in brackets in yy-mm-dd format.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

This feature ensures that data is saved periodically in sensible sized files. This will prevent the computer from crashing and will also ensure that the data is small enough to fit into an Excel spreadsheet

As an example, the user wishes to run the data-logger for seven days recording every minute starting at lunchtime on 12th November 2005. He starts the data logger with the auto-date stamp function enabled. When prompted he gives the filename as test1. In this situation the data logger will run from lunchtime to midnight and then save the first file as test1 (2005-11-12). The data logger then clears and continues for another twenty four hours until midnight the following day. The data is then stored as test1 (2005-11-13). This will continue for seven days when the data-logger will finish.

After this the user will have a sequence of files:

test1 (2005-11-12).txt
test1 (2005-11-13).txt
test1 (2005-11-14).txt

And so on. Combined together they represent all the data over the last seven days. Note that the Rapidox uses the computer clock and date to perform this action, so make sure that they are correct before starting a run.

To view the data in its entirety the user would need to load each file in turn back into Excel to combine.

9.5 *Live Time Graphing Screen*

The Rapidox data-logging package includes a live-time graphing facility that allows you to monitor the progress of your data in a graphical format (see Figure 8). To access the graph check the box labelled 'Show Graph'. The graph will appear in a new window, and can be accessed at any time without disturbing a run that is already in progress. You can select 'Run' and 'Stop' from the Data Logger menu to begin and end data logging, and the window can be minimised to (and restored from) the task bar while logging data.

To close the window and return to the main data-logging page select 'Close Plot' from the File menu or click on the close window button.

The features of the graph window are described below:

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

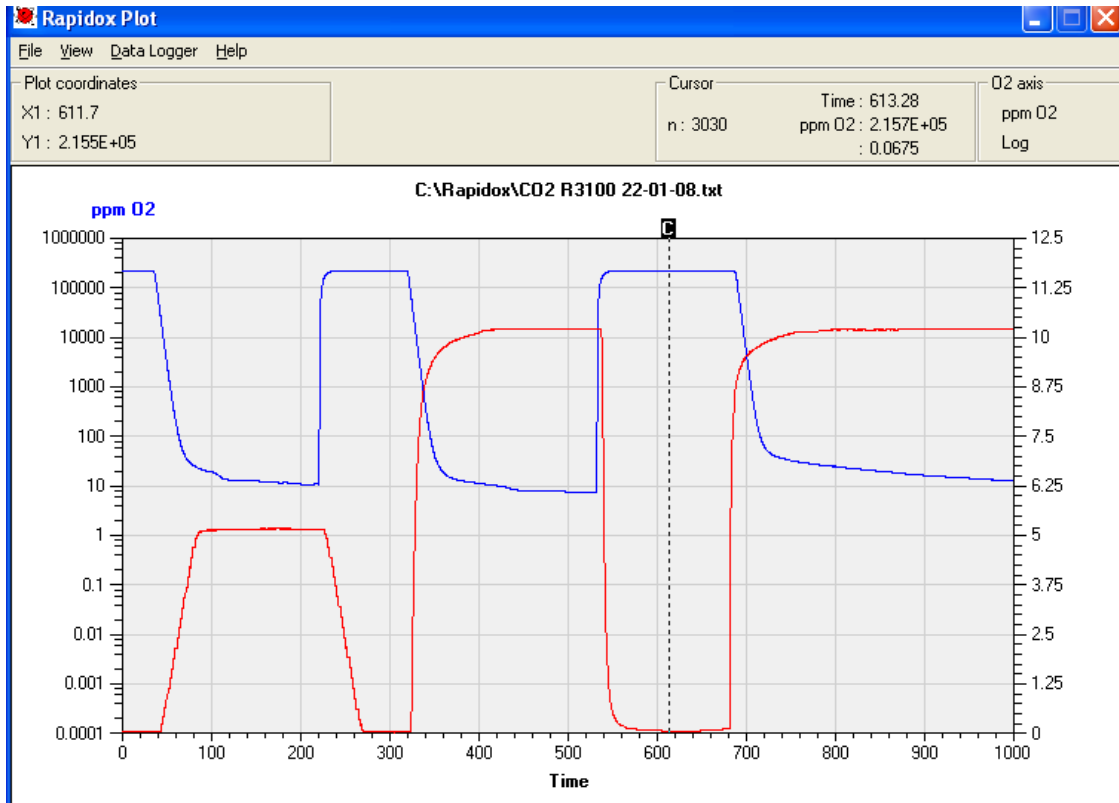


Figure 8: Live-time graphing screen showing O2 (blue) and CO2 (red)

9.6 Main Graph Window

The graph is an XY plot, with time plotted on the X-axis, oxygen plotted on the primary Y-axis (Y1) and a choice of CO₂, temperature (if connected) or internal pressure sensor plotted on the secondary Y-axis (Y2). The X-axis and the two Y-axes auto-scale during data logging so that all data points are shown on the graph.

9.7 Plot Colours

The default colours used on the graph are set to blue for oxygen and red for temperature. To change the colours double-click on the coloured axis label at the top of each axis. A colour palette window will appear (see Figure 9) and a new colour can either be chosen from a colour box, or for more variety, by clicking the 'Define Custom Colors >>' button. Click on 'OK' to select the new colour or 'Cancel' to return to the graph without change.



Figure 9: Plot colour palette menu accessed by double-clicking on the axes titles.

9.8 Graph Titles and Labels

If you want to change the text of the graph axis labels, place the mouse pointer over the text and do a single left click to enter edit mode. The text can then be modified. Similarly, to change the title of the graph, place the mouse pointer over the title and click once to edit. If you choose not to enter a title the graph will display the path and filename of the run as the new title once the run has finished. Note that these changes are only temporary and will be overwritten by the defaults if a new run is started or the graph window is closed and reopened. They are provided so that the plot may be printed with alternative labels.

9.9 Plot Co-ordinates



The box labelled 'Plot co-ordinates' to the upper left of the graph window displays the actual plot co-ordinate value at the mouse pointer. This can be used to get a quick oxygen value from the graph. Simply place the mouse pointer at a place of interest and read the corresponding X1 and Y1 values in the box.

9.10 Last data point

During data acquisition, the box labelled 'Last data point' will appear at the upper middle of the graph window. It displays the last data values read from the analyser.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

9.11 Using the Cursor

Clicking and holding the left mouse button with the pointer over the  at the top of the plot area activates the cursor, which appears as a vertical dashed line on the plot. While keeping the mouse button pressed, you can now move the pointer anywhere in the plot area or on the  in order to move the cursor. The box labelled 'Cursor' to the upper right of the graph window will display actual values for oxygen, temperature, time and the data point number (n) at or immediately to the left of the cursor position. The cursor can be used to investigate actual data values at specific points of interest on the graph.

9.12 Zooming

You can zoom in to any part of the oxygen plot by simply placing the mouse pointer on the new graph start position and then clicking and dragging a new box to re-size the graph. The label on the box to the upper left of the graph window will change to 'Zoom box co-ordinates', and an extra set of co-ordinates, labelled X2 and Y2, will appear, showing the co-ordinates in X and Y units of the second corner of the zoom rectangle as you drag the mouse pointer. The plot will zoom and auto-scale when you release the mouse button. This can be repeated if you wish to zoom in even further. To zoom back to the original size select 'Zoom Full' from the View menu.

Note that although you can use the zoom facility during a live run, the graph will auto-scale to full size with each new data point.

9.13 Y-Axis Graph Units

You can toggle the Y1 oxygen units at any time from percent to ppm and vice versa. Select 'O2 Units' from the View menu and chose either percent or ppm. The current selection is then displayed in the top right box labelled 'O2 Axis'.

9.14 Oxygen Scale

You can display the Y1 oxygen axis in linear or logarithmic format at any time by selecting 'O2 Scale' from the view menu. The current selection is then displayed in the top right box labelled 'O2 Axis'. Note that the zoom function is disabled when you are viewing on a log scale.

9.15 Second Y Axis

The secondary Y axis located on the right hand side of the graph can be used to display either CO₂, temperature taken from the type K thermocouple OR pressure taken from the internal pressure sensor. It is not possible to display CO₂ and temperature / pressure at the same time. The axis is linear and auto-scaling. To select the mode of the secondary axis select 'view' and then 'second axis display'. Choose from 'none', 'CO₂', 'temperature' or 'pressure'.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

9.16 Loading an Old Run

A previously logged data file can be loaded and viewed by selecting 'Open Data File' from the File menu and selecting the appropriate TXT or CSV file. A progress bar is displayed while the data is being imported. Note that very large data files may take several seconds to load. The data is re-graphed and you can zoom, label axes, change colours etc., before printing the graph.

9.17 Printing Graphs

You can print the graph at any time by selecting 'Print Plot' from the File menu. This will bring up the printer dialogue box for your specific printer where you can choose various printing options. Make sure that the printer page is set to landscape to obtain a full size print out.

9.18 Data Logging in the Background

It is possible to begin data logging and then minimise the windows to continue working with another application. To minimise the graph simply click on the minimise button on the blue title bar at the top of the window. You can then use the ALT + TAB keys to take you to other programmes already running. To return to the graph simply maximise from the start menu bar or press ALT + TAB again. If the graph does not redraw immediately select 'Zoom Full' from the View menu to redraw.

9.19 Pausing the Data Logging

You can pause the data-logging at any time during the run by selecting the 'data logger' menu and selecting 'pause'. Repeat the action to continue, noting that the live graph will draw a straight line between the paused points to keep continuity of the axes. The clock keeps ticking during the pause period.

If you decide to access the menu of the Rapidox using the front keypad during data logging, then the software will pause automatically. A message appears on the screen informing the user that the unit is being accessed from the keypad. Once the menu has been exited, the software will continue data logging from where it left off.

9.20 Changing the Data Logging Parameters Mid-run

Once the data logging has begun you may change the sample interval time by pausing the data logger and then entering a new value for the time interval. The data logger can then be resumed with the new values in place. Note that you can not change units (e.g. seconds to hours) once logging has started. If you originally selected seconds then you may change the current value to a new value between 1 and 3600 seconds, if you originally selected minutes then you may change between

0.02 and 360 and if you selected hours you may change between 0.01 and 6 hours. Note it is not possible to modify the original total length of time that the data logging will run for once a run has commenced.

9.21 Working with Spreadsheets

The data-logger saves data files in a standard comma separated ASCII text format which can be readily imported into spreadsheet programmes such as MS Excel, in order to produce plots and reports as desired. For specific information on how to import text files into your spreadsheet programme please refer to the help guide supplied with the programme.

Data is saved in comma separated value format, with a '.txt' file extension as the initial programme default. However, when entering the file name, you can instead select a '.csv' extension: the programme will register the last used file extension as the new default. The '.csv' extension is recognised by MS Excel, so that opening the file will automatically run MS Excel, and this may be of benefit if your regional decimal separator is period '.' rather than comma ','. However, if your decimal separator is comma, you should continue to use the '.txt' extension and open the file explicitly from within your spreadsheet programme, defining the field delimiter as 'comma' where appropriate.

9.22 Disaster Recovery

To prevent catastrophic loss of important data during a computer crash or power failure, the data is automatically saved point by point in a temporary file called 'Rapidox temporary data file.txt'. This file is located in the same directory as the main Rapidox programme itself and can be renamed or copied to recover data that would otherwise be lost. Note that this file is overwritten each time 'Run' is selected from the Data Logger menu so make sure all data is recovered successfully before starting another run.

Note that during a run using the 'auto date stamped' feature the temporary data file is wiped clean as soon as the previous data set has been saved successfully. In the case of a crash the temporary data file should be used to recover the last day's worth of data that was not saved to the hard disc.

9.23 Diagnostics

The Rapidox software includes a diagnostics page that is accessed from the tab labelled 'Diagnostics'. This screen will display various values and settings that are operating inside your machine. There is no editing possible on this page – it is purely for information and to enable technical support help you should you experience difficulties with your machine. You may be asked to record values from this page if trouble shooting is required.

10. Troubleshooting

- Q: The Rapidox says 'sensor heating' but won't begin measuring.
A: Contact Cambridge Sensotec for advice. It is possible that the sensor has failed and needs replacing
- Q: The Rapidox won't power up at all.
A: There are fuses located on the power socket on both live and neutral lines. These are standard 20mm (1A for 240V versions, 2A for 110V) fuses available from a supplier such as RS Components.
- Q: The Rapidox gives strange readings that are way off the expected values.
A: Check the software to make sure that the 'Operating pressure' is correct otherwise this will introduce a multiplying error. Also check to make sure which two calibration gases are selected. Are they the same as the actual gases you used to perform the calibration? If not you can change their values using the software.
- Q: The sensor does not read 20.9 - 21.0% in air (actual value is 20.95%).
A: If the room air is very humid, it will slightly affect the observed measurement or the sensor may have drifted slightly because of natural ageing. If you are using air as a calibration point then simply do a quick re-calibration in the air to compensate for this.
- Q: I messed up the calibration procedure and the analyser is not working properly.
A: Return the box to the factory defaults using the communications software, by selecting 'Default Configuration' followed by 'Write Configuration to Analyser' from the File menu. Now try re-calibrating the Rapidox.
- Q: The date and time information on the RS232 is incorrect.
A: The date, time and other features are user-programmable via the configuration software. Make sure that they are correct on the PC you are using before attempting to reprogram the Rapidox.
- Q: The software will not talk to the Rapidox.
A: Make sure that you are using the correct cable, as supplied (pin 2 to pin 2 etc). A crossed RS232 cable (pin 2 to pin 3 etc.,) will not work. Make sure that your COM ports are recognised by your computer. Check in your Windows device manager to see if there are any conflicts. If you have an internal modem fixed to your PC you may experience difficulties using this software. Contact Cambridge Sensotec for further advice.
- Q: I selected 'Write to the Analyser' and now the Rapidox is way off calibration.
A: Only select 'Write to the Analyser' once all the values are correctly entered in the boxes on the right. The best procedure is to 'Read Analyser Configuration' and then press 'Copy' so the values in the boxes are the same as those stored in the Rapidox memory. You can then edit these values and then select 'Write to the Analyser' when finished.

Rapidox 3100A Dual Gas Oxygen/CO₂ Analyser Instruction Manual

Q: How do I get back to the factory calibration for my instrument?

A: Select 'Load Configuration File' from the File menu and look for the rxc file on your CD. Select this file and then select 'Write to the Analyser'. This will load the factory calibration back into the Rapidox. Alternatively you can load a standard default configuration any time using the 'Load Default' option on the File menu. This configuration will not be perfect for your analyser but will be good enough to get you started again.

11. Warranty

The Rapidox 3100 analyser has been carefully tested and inspected before shipment and is guaranteed to be free from defective materials and workmanship for a period of twelve months from date of purchase. The sensor head is replaceable and has a life expectancy of up to 35,000 hours. However, if the analysis gas contains corrosive gases or large quantities of particulates, sensor life may be shortened. In the case of the latter, it is normally possible to insert a filter prior to the sensor head to remove the particulate material.

11.1 Conditions of Warranty:

- 1) This warranty is in addition to and does not affect any statutory rights of consumer purchasers. This warranty is valid worldwide on a back to base basis.
- 2) This warranty covers breakdowns due to design or manufacturing faults; it does not apply to damage, however caused, wear and tear, neglect, unauthorised adjustment or repair, or any items of limited natural life.
- 3) In the event of failure, please take the following action:
 - a) Refer to the "Troubleshooting" section of your instruction manual to identify and possibly correct the problem.
 - b) If the fault cannot be resolved, please contact the Cambridge Sensotec service and repair centre at the address given on the cover of the manual.
- 4) The warranty period applicable shall be 12 months from the date of purchase and delivery.

Rapidox CERTIFICATE of CALIBRATION

Date:

Rapidox Serial number:

Calibration Constant A

Calibration Constant B

Calibration Gas 1

Calibration Gas 2

Configuration Filename

CO₂ Calibration Check: Gas 5.0% reading:

Calibrated by:

Signed:

Cambridge Sensotec Rapidox 3100 Oxygen Analyser Instruction Manual